


Pro D·I·G·I·T·A·L

Quick Start Guide

Item #626972




This is a reference guide for operating the ProDIGITAL line of handhelds. Refer to the User Manual for more information.

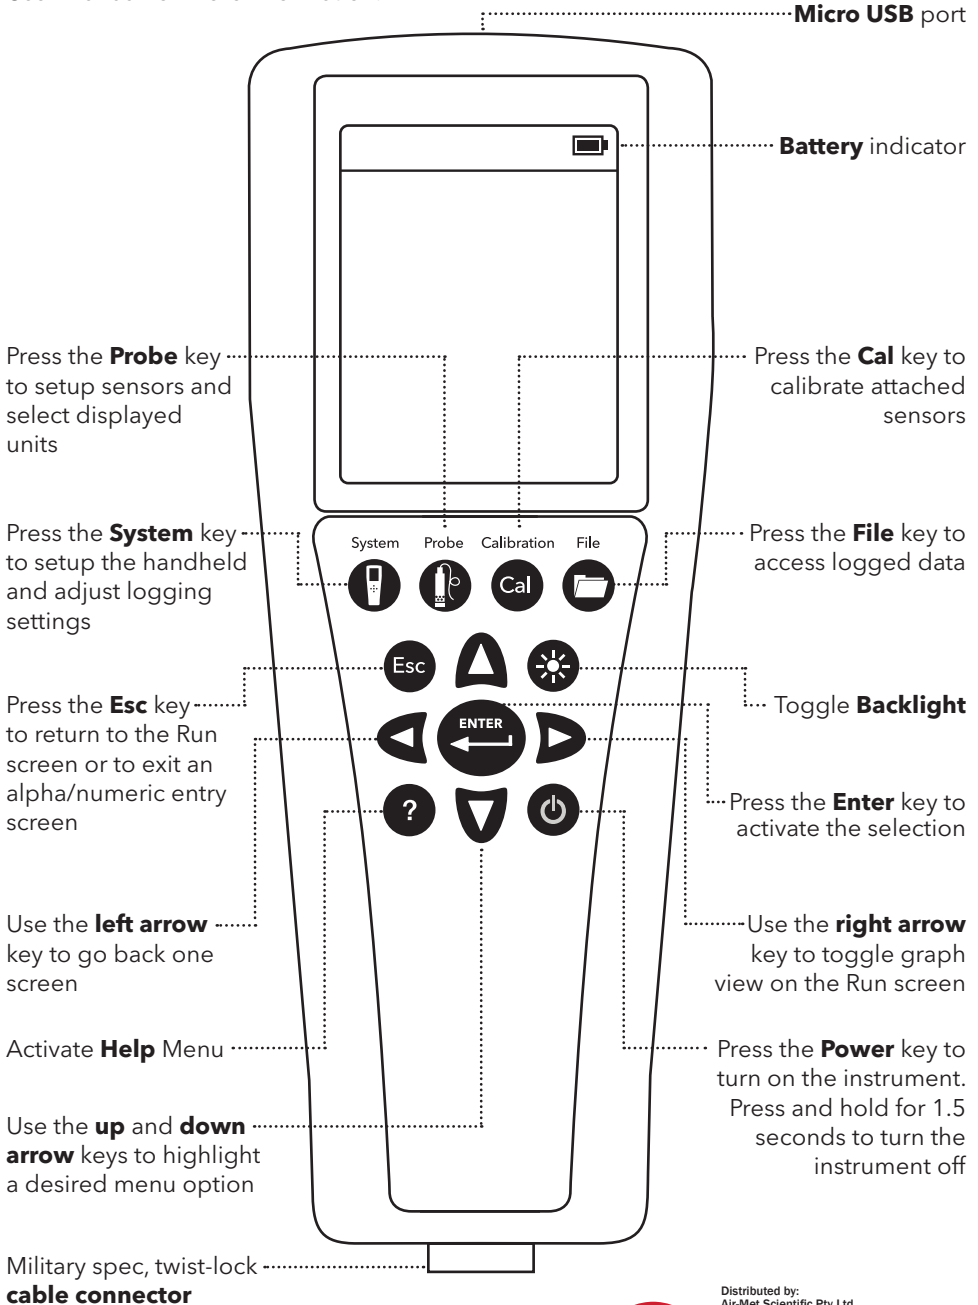



Distributed by:
Air-Met Scientific Pty Ltd
Air-Met Sales/Service
P: 1800 000 744
F: 1800 000 774
E: sales@airmet.com.au


Air-Met Rental
P: 1300 137 067
E: hire@airmet.com.au
W: www.airmet.com.au

Setting Up


 Charge the battery by connecting the handheld to an AC power supply or USB connector using the micro USB cable. Ensure all components are dry when charging. A full charge takes approximately 9 hours.

 Make sure the **date/time** is correct and set the **logging mode** (Single or Continuous).

 Setup sensor parameters and select **units displayed** on the Run and Data View screens.

 **Calibrate sensors** prior to taking measurements; sensor-specific calibration instructions can be found in the User Manual.

Taking Measurements

 Insert the probe into the sample and briefly move it up and down to release any air bubbles. Allow measurements to stabilize and press the Enter key to **log data**. To stop Continuous logging, simply press the Enter key again.

Data Management

 Press the File key to **view, delete, or backup** logged data. Data can be filtered by date/time and by the user-created Site and/or Data ID.

 Transfer data to your PC using **KorDSS Software**. Make sure the instrument driver and software are installed from the included USB flash drive or from **YSI.com**.

1. Open KorDSS Software.
2. Use the micro USB cable to connect the handheld to the PC.
3. Power on the handheld; there may be a short delay before it shows up in the software.
4. Select the handheld under the **Instrument Connection Panel** and click Connect.
5. Click **Start Download from Device**.
6. After data download, click **View Logged Data** to view, print, and export data files from KorDSS.